

Thermo Scientific Orion Fuse Kit for the 2100 Series Process Monitors

General Information


The fuse kit is supplied in the options kit that is shipped with all 2100 series process monitors. The fuse kit contains 2 each of the following fuse ratings:

AC Voltage	Fuse Rating
115 V	200 mA, 250 V, fast acting
230 V	100 mA, 250 V, fast acting

Fuse Installation

1. Select the correct fuse from the fuse kit. The fuses are clearly labeled with the appropriate voltages for your system – either 115 V or 230 V.

Be sure to throw away the fuses with the voltage that is not needed.
2. Insert the fuse into the fuse holder cap.
3. Install the fuse holder cap into the fuse holder by aligning the pin on the cap with the notch in the holder.
4. Push in the fuse as far as possible. Secure the fuse by turning it 1/4 to the right.

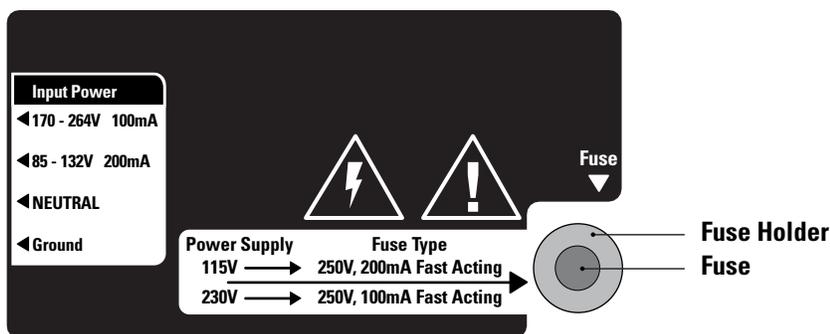

Ordering Information

Cat. No.	Description
2100FK115	Fuse kit assembly, 115 V
2100FK230	Fuse kit assembly, 230 V

©2009 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries.



Process Water Instruments

North America
166 Cummings Center
Beverly, MA 01915 USA
Toll Free: 1-800-225-1480
Tel: 1-978-232-6000
Dom. Fax: 1-978-232-6015
Int'l Fax: 978-232-6031

Europe
P.O. Box 254, 3860 AG Nijkerk
Wallerstraat 125K, 3862 BN
Nijkerk, Netherlands
Tel: (31) 033-2463887
Fax: (31) 033-2460832

Asia Pacific
Blk 55, Ayer Rajah Crescent
#04-16/24, Singapore 139949
Tel: 65-6778-6876
Fax: 65-6773-0836

www.thermo.com/processwater

